




GENERAL SECUREMENT DEVICES

Grip-Lok® is a portfolio of versatile adhesive-based devices that promotes patient comfort and secures a variety of tubes, lines, and catheters.

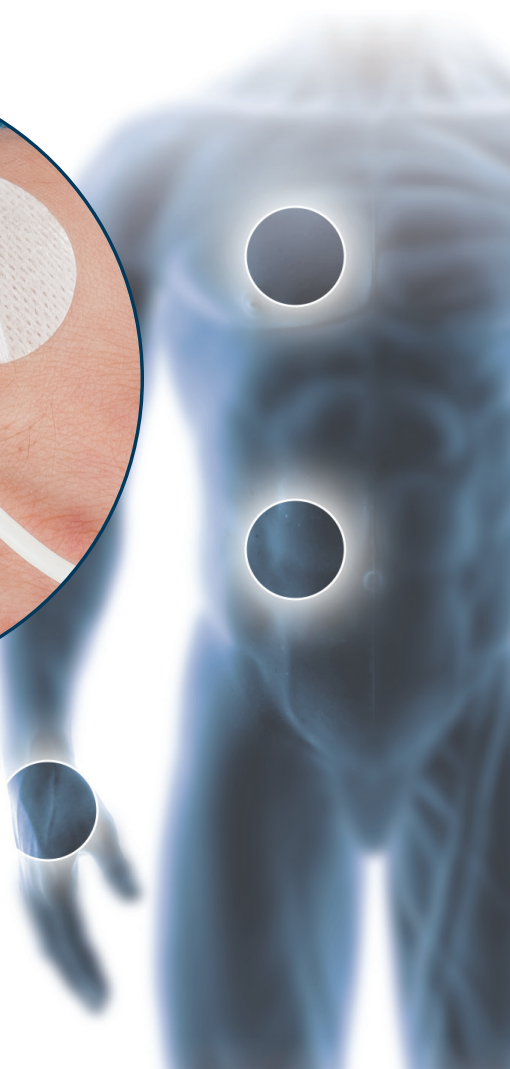

Product Details

- Secures a wide variety of tube sizes (see chart)
- Meets INS guidelines for engineered securement¹
- Not made with natural rubber latex

SKU Number	Description	Quantity	Size Range	Catheter/Device Materials
3200S	Small Securement Device	100/Bx	4.5 – 13.5 FR	PVC, Polyethylene, Polyurethane
3300M	Medium Securement Device	100/Bx	9 – 24 FR	PVC, Polyethylene, Polyurethane
3400L	Large Securement Device	100/Bx	16 – 40 FR	PVC, Polyethylene, Polyurethane
3300MWA	Medium Wide Securement Device	100/Bx	16 – 40 FR	Silicone, PVC, Polyethylene, Polyurethane

Performance

SKU Number	Average Minimum Dislodgement Force ²	Average Minimum Resistance to Peel ³
3200S	2.5lbf / 11.2 N	2.3lbf / 10.2 N
3300M	6.2lbf / 27.6 N	3.0lbf / 13.3 N
3400L	9.5lbf / 42.3 N	3.9lbf / 17.3 N
3300MWA	11.2lbf ⁴ / 49.8 N	4.2lbf ⁵ / 18.7 N

Patient Comfort

- Developed with medical grade, hypoallergenic adhesive
- Flexible materials and a low profile

Ease-of-Use

- Similar application methods used throughout portfolio
- Hook-and-loop tab allows access to the catheter, line, or tube
- Large and glove-friendly peel-away liners

Grip-Lok General Securement can be used with the following devices⁶:

Hypoallergenic skin
contact adhesives

Adhesive areas
grip without plastic
locking mechanisms

Large peel-away
liners for
easy application

Hook-and-loop technology
allows access to the line

Breathable, nonwoven bandage
material resists moisture⁷

Chest Tubes

PEG/PEJ Tubes

IV Tubing



For more information, contact your sales representative
or visit <http://tidiproductions.com/grip-lok/>
For U.S. and foreign patent information,
visit go.tidiproductions.com/patents

References

1. Infusion Nurses Society (2016), Infusion Therapy Standards of Practice. Journal of Infusion Nursing, 39 (1S), S73
2. Dislodgement Force is defined as the amount of force from either an axial or side load force to remove the patient device from the securement device. Data on file.
3. Resistance to Peel is defined by the amount of force in the perpendicular direction to remove the patient device from the securement device. Data on file.
4. Silicone material resisted to 4.4 lbf / 19.6 N
5. Silicone material resisted to 3.1 lbf / 13.8 N
6. In accordance with the tubing size and material chart
7. Data on file